

Accurate Optical Lattice Clock with ^{87}Sr Atoms

Rodolphe Le Targat, Xavier Baillard, Mathilde Fouché, Anders Brusch, Olivier Tcherbakoff,
Giovanni D. Rovera, and Pierre Lemonde*

LNE-SYRTE, Observatoire de Paris 61, Avenue de l'Observatoire, 75014 Paris, France

(Received 23 May 2006; published 26 September 2006)

We report a frequency measurement of the $^1S_0 - ^3P_0$ transition of ^{87}Sr atoms in an optical lattice clock. The frequency is determined to be $429\,228\,004\,229\,879(5)$ Hz with a fractional uncertainty that is comparable to state-of-the-art optical clocks with neutral atoms in free fall. The two previous measurements of this transition were found to disagree by about 2×10^{-13} , i.e., almost 4 times the combined error bar and 4 to 5 orders of magnitude larger than the claimed ultimate accuracy of this new type of clocks. Our measurement is in agreement with one of these two values and essentially resolves this discrepancy.

DOI: [10.1103/PhysRevLett.97.130801](https://doi.org/10.1103/PhysRevLett.97.130801)

PACS numbers: 06.30.Ft, 32.80.-t, 42.50.Hz, 42.62.Fi

Recent advances in the field of optical frequency metrology make measurements with a fractional accuracy of 10^{-17} or better a realistic short term goal [1]. Among other possible applications (e.g., a redefinition of the SI second, optical very long baseline interferometry in space, direct mapping of Earth's gravity using the gravitational redshift, ...), a very interesting prospect with measurements at that level is a reproducible test of Einstein equivalence principle by the repeated determination of the frequency ratio of different atomic and molecular transitions [2–7]. The topicality of such a test has recently been renewed by measurements at the cosmological scale which seem to indicate a slow variation of the electron to proton mass ratio [8]. The richness of the test directly depends on the performance of the clocks that are used but also on the variety of clock transitions and atomic species on which high accuracy frequency standards are based.

In that context, optical lattice clocks are expected to play a central role in the future of this field. They use a large number of atoms confined in the Lamb-Dicke regime by an optical lattice in which the first order perturbation of the clock transition cancels [9]. Because of lattice confinement, motional effects, which set a severe limitation to standards with neutral atoms in free fall [10,11], essentially vanish [12]. This gives hope for a ultimate fractional accuracy better than 10^{-17} . On the other hand, the large number of atoms in an optical lattice clock in principle opens the way to a short term fractional frequency stability significantly better than $10^{-15}\tau^{-1/2}$ with τ the averaging time in seconds. In this regime the coherence time of the laser frequency locked to the clock transition would be several seconds, possibly tens of seconds [13]. Such a long coherence time could, for instance, be used to reduce the width of the optical resonances in single ion clocks down to or below the 0.1 Hz range opening new prospects for these devices also. Finally, the optical lattice clock scheme is in principle applicable to a large number of atomic species (Sr, Yb, Hg, Ca, Mg, ...) which is a key feature for the fundamental test discussed above. It is then particularly

problematic that the frequency delivered by the first two evaluated optical lattice clocks, which both use ^{87}Sr , disagree by about 2×10^{-13} [14,15], i.e., 3.5 times the combined error bar of the measurements.

We report here a third independent measurement of the $^1S_0 - ^3P_0$ transition of ^{87}Sr in an optical lattice clock. Our measurement turns out to agree with the one of Ref. [15]. The trapping potential used here is significantly larger as compared to both previous experiments. We operate the optical lattice clock with trapping depths ranging from $U_0 = 100E_r$ to $U_0 = 900E_r$, where E_r is the recoil energy associated to the absorption or emission of a lattice photon ($E_r/h = 3.58$ kHz). We demonstrate that at such large lattice depths, the residual light shift of the clock transition is controlled at the Hz level, i.e., in the range of a few 10^{-7} of the individual light shift of both involved atomic states. This rules out the explanation of the disagreement between previous experiments by an unexpected large frequency shift which would arise in this new type of clock. Including

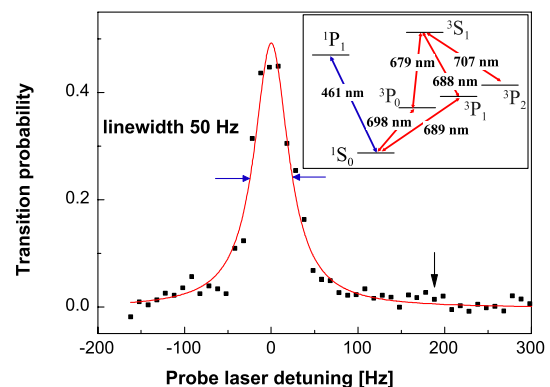


FIG. 1 (color online). Atomic carrier resonance at 698 nm for a probe time of 15 ms, a power of $3 \mu\text{W}$ and lattice depth $U_0 = 170E_r$. The vertical arrow is at a detuning corresponding to the transverse oscillation frequency for this value of U_0 : $\nu_{\perp} = 186$ Hz. The solid line is a fit of the experimental data by a Lorentzian. Inset: relevant energy levels of Sr.

the evaluation of the other systematic effects, the fractional accuracy of the clock is 1.2×10^{-14} , comparable to state-of-the-art optical frequency standards using neutral atoms in free fall [5,11].

The Sr optical lattice clock has been described in Ref. [16] and we only briefly recall the main features of its operation time sequence. We first load atoms in the vertical 1D optical lattice operated at its maximum depth, presently 150 μK . The lattice beam is focused to a 90 μm $1/e^2$ waist radius and goes through a cloud of cold atoms at 2 mK that is produced by a magneto-optical trap (MOT) based on the $^1S_0 - ^1P_1$ transition (see the relevant energy levels in Fig. 1). Atoms at the center of the lattice beam are drained to the 3P_0 and 3P_2 metastable states by a two-photon optical pumping scheme using the transitions at 688 nm and 689 nm. This leads to a continuous loading of the lattice at a rate of a few 10^4 atoms/s. After typically 500 ms of loading time, the MOT and drain lasers are switched off. Atoms are repumped back to the 1S_0 ground state, and cooled down to about 10 μK in 60 ms using the narrow $^1S_0 - ^3P_1$ intercombination transition at 689 nm. Next, the lattice depth is ramped down in 1 ms and the clock transition is probed by a beam at 698 nm from an interference-filter stabilized extended cavity diode laser [17]. Its emission spectrum is narrowed by Pound-Drever-Hall locking to an ultrastable cavity [18,19]. The probe beam is overlapped with the dipole trap and has a waist radius of 210 μm . The transition probability to 3P_0 is finally measured by detecting successively the populations of both 1S_0 and 3P_0 states.

The excitation spectrum at 698 nm consists in a narrow carrier at the clock transition frequency that is surrounded by motional sidebands detuned by the lattice oscillation frequencies. The carrier is displayed in Fig. 1. It has a width of 50 Hz, for a probe time of 15 ms and a laser power of 3 μW . The corresponding line Q factor is about 10^{13} . We observed no dependence of the linewidth on the depth of the trapping potential (the resonance of Fig. 1 was for $U_0 = 170E_r$). Depending on the depth of the lattice during the probe pulse the longitudinal oscillation frequency ranges from 70 kHz to 210 kHz, 3 orders of magnitude larger than the width of the resonance. In addition, the corresponding sidebands are reduced by a factor η^2 [20], with η the Lamb-Dicke parameter ranging from 0.1 to 0.03 here. The frequency pulling of the carrier by the longitudinal sidebands is therefore totally negligible. The transverse confinement of the atoms is much weaker than the longitudinal one and leads to an oscillation frequency between 140 Hz and 410 Hz depending on the lattice depth. Excitation of the transverse sidebands is possible due to the nonzero transverse content of the probe wave-vector distribution. This content orthogonal to the lattice results from the imperfection of the probe and lattice alignment, wave front aberrations, and diffraction (the divergence of the probe beam is 1 mrad). However, as can be seen in

Fig. 1, transverse sidebands do not emerge from the noise in the experimental spectrum and are at least 20 times smaller than the carrier. The corresponding line frequency pulling is less than 1 Hz.

The frequency measurement chain is depicted in Fig. 2. The probe beam frequency is locked to the atomic transition by alternately probing both sides of the carrier resonance. The difference between two successive measurements of the transition probability gives the error signal that is digitally integrated to servo control the frequency of an acousto-optic modulator (AOM) used to bridge the detuning between the atomic transition and the ultrastable cavity. The cavity frequency is continuously measured by means of a femtosecond frequency comb relative to a 1 GHz signal [21,22]. The latter is provided by a cryogenic sapphire oscillator [23] that is locked to a H maser and referenced to the SI second by the cesium fountain clock FO2 with a relative uncertainty better than 6×10^{-16} [24]. The fractional Allan standard deviation of the measurement is $6 \times 10^{-14} \tau^{-1/2}$ and is displayed on Fig. 3. The frequency resolution is therefore 1 Hz (or 2.3×10^{-15} in fractional units) after about 10 minutes of integration time. The main contributors to the measurement noise are the femtosecond frequency comb and the strontium clock with roughly equal weights [25].

The residual first order Zeeman effect is the main source of uncertainty in our measurement. Both clock levels of total internal angular momentum $F = 9/2$ have different Landé factors which correspond to a frequency shift of $-0.18m_F$ Hz/mG and $-0.08m_F$ Hz/mG for 1S_0 and 3P_0 , respectively, with m_F the magnetic number. The measurements are performed at zero magnetic field. Three pairs of Helmholtz coils surround the vacuum chamber and are used to compensate for the environmental field by minimizing the width of the atomic carrier resonance. The cancellation is performed to within 10 mG, limited by

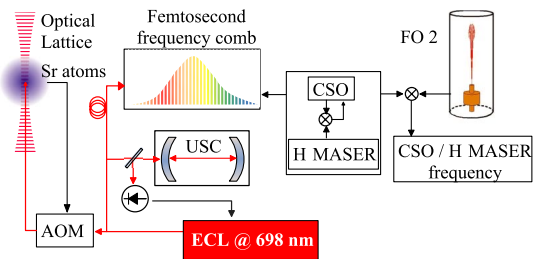


FIG. 2 (color online). Scheme of the frequency measurement chain: a 698 nm extended cavity laser (ECL) is locked to an ultrastable cavity (USC) by a Pound-Drever-Hall servo loop. The error signal generated by probing the atoms in the optical lattice is fed back to control the frequency of the acousto-optic modulator (AOM). The femtosecond frequency comb is used to measure the cavity resonance frequency relative to a cryogenic sapphire oscillator (CSO) locked to a hydrogen maser. The measurement of the frequency of this oscillator by the fountain clock FO2 enables referencing to the SI second.

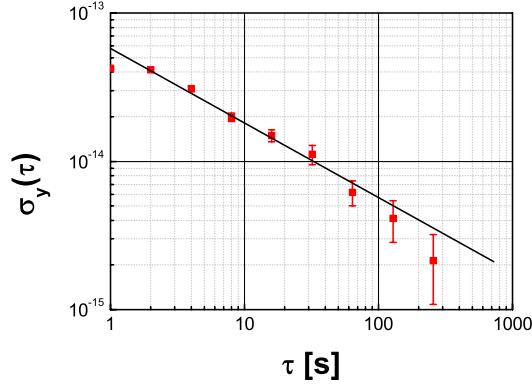


FIG. 3 (color online). Allan deviation of the frequency measurements. The straight line is a fit by a $\tau^{-1/2}$ law.

environmental fluctuations. The residual field may result in a systematic frequency shift if there is an unbalance between the Zeeman sublevels populations or an asymmetry of the probe laser polarization with respect to the direction of that field. The population asymmetry is tested by measuring the clock frequency as a function of the depth of the servo-loop frequency modulation. The results of this experiment are shown in Fig. 4(a) for various values of the angle formed by the probe laser and the lattice beam polarizations showing no clear dependence of the clock

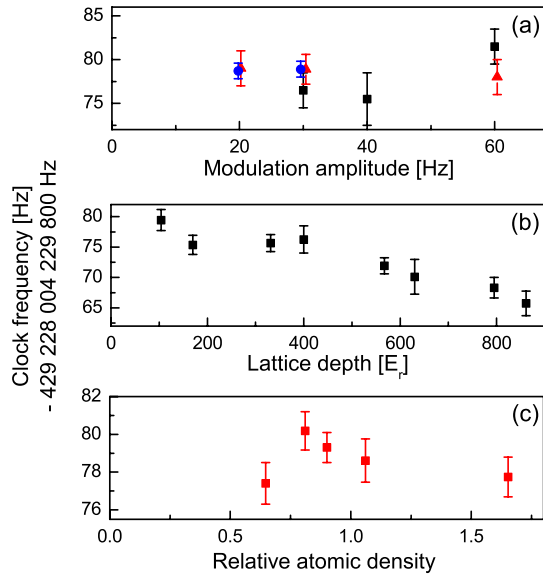


FIG. 4 (color online). (a) Clock frequency as a function of the peak to peak amplitude of the frequency modulation applied for the frequency lock to the atomic resonance. A modulation amplitude of 25 Hz corresponds to locking at half maximum of the resonance. Measurements are performed for various values of α , the angle formed by the lattice and probe beam polarizations. Both polarizations are linear. \blacksquare : $\alpha = 0$, \blacktriangle : $\alpha = \pi/2$, \bullet : $\alpha = \pi/4$. (b) Clock frequency as a function of the lattice depth. (c): Clock frequency vs atomic density. For all three plots, the error bars include the statistical uncertainty only.

frequency on these parameters. We conservatively assign an uncertainty of 5 Hz to the first order Zeeman effect. All the measurements reported in Fig. 4(a) fit within this error bar which also corresponds to the maximum shift for a stray 10 mG field. This present limitation to our accuracy budget is purely technical and can certainly be improved by orders of magnitude by resolving the Zeeman structure and using spin-polarized atoms.

The lattice wavelength control is presently performed with a commercial wave meter which exhibits long term fluctuations of the order of 10^{-3} nm at 813 nm. Tuning of the lattice to the exact point where the first order light shift cancels is therefore limited to that level and all measurements are performed by interleaving sequences with different lattice depths [16]. In Fig. 4(b) is shown the clock frequency as a function of the lattice depth. The detuning with respect to the magic wavelength deduced from this particular measurement is 1.1×10^{-3} nm. At the average lattice depth $U_0 = 400E_r$, the differential light shift is 4.5(9) Hz with an uncertainty which corresponds to 6×10^{-7} of the individual shift of both clock states. Note that this evaluation phenomenologically accounts for all contributors to the atomic dynamic polarizability including the higher order multipolar terms and the residual vector and tensor terms in the actual polarization and magnetic state configuration [26]: all these terms lead to frequency shifts that are proportional to U_0 . The frequency shift due to the atomic hyperpolarizability, which scales as U_0^2 , is evaluated by combining the present measurements with those of Ref. [16]. This leads to a correction of the measurements by 0.6 Hz at $U_0 = 400E_r$ with an uncertainty equal to the correction.

We have also measured the clock frequency as a function of the atomic density to check for a possible frequency shift due to cold collisions in our unpolarized fermionic sample. The atomic density is varied by changing the MOT beams intensity. The results are plotted in Fig. 4(c) and

TABLE I. Uncertainty budget (all numbers are in Hz). The shifts due to the lattice are given at $U_0 = 400E_r$ which is our average lattice depth for this measurement.

Systematic effects	Correction	Uncertainty
First order Zeeman shift	0	5
Lattice ac Stark shift	4.5	0.9
Lattice 2nd order Stark shift ^a	0.6	0.6
Line pulling by motional sidebands	0	1
Cold collisions	1	1
Probe ac Stark shift	0	$\ll 1$
Blackbody radiation shift	2.4	$\ll 1$
FO2 fountain accuracy	0	$\ll 1$
Total	8.5	5.3

^aThese numbers result from the data of Ref. [16] combined with the new measurements performed here.

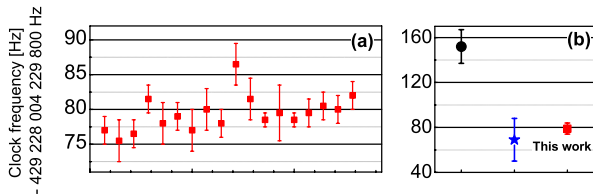


FIG. 5 (color online). (a) Measurements of the clock transition with their individual statistical error bar. The average of these points is 429 228 004 229 879.4 Hz with a statistical uncertainty of 0.45 Hz [$\chi^2/(N-1) = 1.0$ with N the number of experimental points]. The uncertainty on systematic effects is 5 Hz. (b) Reported measurements of the $^1S_0 - ^3P_0$ transition of ^{87}Sr . ●: Ref. [14], ★: Ref. [15], ■: this work.

lead to a correction of the clock frequency of 1(1) Hz at the average atomic density of about 10^{11} at/cm³.

The blackbody radiation shift is -2.4 Hz at a temperature of 293 K, as calculated in Ref. [9]. This type of calculation is known to be accurate at the percent level [27,28]. The contribution to that shift of the Sr oven ($T = 500$ °C) is negligible at the present level of accuracy. Its distance from the atoms is about 60 cm for a diameter of 4 mm set by diaphragms at room temperature.

Finally, we also computed the ac Stark shift due to the probe itself. For a probe laser power of 3 μW , the calculated light shift is about 90 mHz, dominated by the contribution of the $^3P_0 - ^3S_1$ transition.

The accuracy budget of the Sr optical clock is summarized in Table I and gives a total systematic uncertainty of 5 Hz. The weighted average of our measurements which are plotted in Fig. 5(a) is 429 228 004 229 879.4 Hz with a statistical uncertainty of 0.5 Hz. In Fig. 5(b) are shown the result of this new measurement together with the two previously published values of Ref. [14,15]. Our measurement is in excellent agreement with the one of Ref. [15]. This agreement is a confirmation that optical lattice clocks can indeed operate at a high level of accuracy.

Today this level is comparable to state-of-the-art optical clocks with neutral atoms in free fall [5,11] with obviously large room for improvement. By polarizing the atoms and using a small bias magnetic field, we hope to be able to decrease by orders of magnitude the uncertainty due to the linear Zeeman effect which is presently the main contributor to the measurement uncertainty. The evaluation of the other effects will take advantage of the unprecedented versatility of this new type of clock. A large number of operation parameters can be varied such as the trapping depth and configuration (polarization of the trapping laser, 1D or 3D lattice), the probe polarization, the atom number, the interrogation scheme (Rabi or Ramsey), and duration,

etc. This will be of great value for untangling the various physical effects that will contribute to a largely improved uncertainty budget.

We thank A. Clairon and S. Bize for useful comments on the manuscript and together with G. Santarelli, F. Chapelet, and M. Tobar for their work on the FO2 fountain and cryogenic oscillator. SYRTE is Unité Associée au CNRS (No. UMR 8630) and a member of IFRAF (Institut Francilien de Recherche sur les Atomes Froids). This work is supported by CNES and DGA.

*Electronic address: pierre.lemonde@obspm.fr

- [1] L. Hollberg *et al.*, J. Phys. B **38**, S469 (2005).
- [2] J.-P. Uzan, Rev. Mod. Phys. **75**, 403 (2003).
- [3] H. Marion *et al.*, Phys. Rev. Lett. **90**, 150801 (2003).
- [4] S. Bize *et al.*, Phys. Rev. Lett. **90**, 150802 (2003).
- [5] M. Fischer *et al.*, Phys. Rev. Lett. **92**, 230802 (2004).
- [6] E. Peik *et al.*, Phys. Rev. Lett. **93**, 170801 (2004).
- [7] R. Srianand, H. Chand, P. Petitjean, and B. Aracil, Phys. Rev. Lett. **92**, 121302 (2004).
- [8] E. Reinhold *et al.*, Phys. Rev. Lett. **96**, 151101 (2006).
- [9] H. Katori, M. Takamoto, V.G. Pal'chikov, and V.D. Ovsiannikov, Phys. Rev. Lett. **91**, 173005 (2003).
- [10] R. Li and K. Gibble, Metrologia **41**, 376 (2004).
- [11] U. Sterr *et al.*, C.R. Physique **5**, 845 (2004).
- [12] P. Lemonde and P. Wolf, Phys. Rev. A **72**, 033409 (2005).
- [13] This implies that the time constant of this servo-loop be shorter than the coherence time of the free-running probe laser.
- [14] M. Takamoto, F.-L. Hong, R. Higashi, and H. Katori, Nature (London) **435**, 321 (2005).
- [15] A.D. Ludlow *et al.*, Phys. Rev. Lett. **96**, 033003 (2006).
- [16] A. Brusch *et al.*, Phys. Rev. Lett. **96**, 103003 (2006).
- [17] X. Baillard *et al.*, physics/0605046 [Opt. Comm. (to be published)].
- [18] R. W. P. Drever *et al.*, Appl. Phys. B **31**, 97 (1983).
- [19] A. Quesada *et al.*, J. Opt. B **5**, S150 (2003).
- [20] D. Leibfried, R. Blatt, C. Monroe, and D. Wineland, Rev. Mod. Phys. **75**, 281 (2003).
- [21] R. Holzwarth *et al.*, Phys. Rev. Lett. **85**, 2264 (2000).
- [22] D.J. Jones *et al.*, Science **288**, 635 (2000).
- [23] D. Chambon *et al.*, Rev. Sci. Instrum. **76**, 094704 (2005).
- [24] S. Bize *et al.*, C.R. Physique **5**, 829 (2004).
- [25] The femtosecond frequency comb measurements average down as $\tau^{-1/2}$ due to a 200 ms dead time between two successive measurements.
- [26] V. Ovsiannikov, V. Pal'chikov, H. Katori, and M. Takamoto, Quantum Electron. **36**, 3 (2006).
- [27] E.J. Angstmann, V.A. Dzuba, and V.V. Flambaum, Phys. Rev. Lett. **97**, 040802 (2006).
- [28] K. Beloy, U.I. Safronova, and A. Derevianko, Phys. Rev. Lett. **97**, 040801 (2006).